

SRS

Spectral Reflectance Sensor

Operator's Manual



Decagon Devices, Inc.

Version: June 12, 2013 — 14:00:40

Decagon Devices, Inc.
2365 NE Hopkins Court
Pullman WA 99163

Phone: 509-332-5600

Fax: 509-332-5504

Website: www.decagon.com

Email: support@decagon.com or sales@decagon.com

Trademarks

©2007-2013 Decagon Devices, Inc.

All Rights Reserved

Contents

1	Introduction	1
1.1	Customer Support	1
1.2	About This Manual	2
1.3	Warranty	2
1.4	Seller's Liability	2
2	About SRS	3
2.1	Overview	3
2.2	Specifications	4
3	Theory	6
3.1	Normalized Difference Vegetation Index (NDVI)	6
3.2	Fractional Interception of Photosynthetically Active Radiation	8
3.3	Canopy Phenology	10
3.4	Photochemical Reflectance Index (PRI)	11
3.5	Sun-Sensor-Surface Geometry Considerations	12
3.6	Calculating Percent Reflectance from Paired Up and Down Looking Sensors	14
4	Connecting the SRS	19
4.1	Connecting to Decagon Data Logger	19
4.2	3.5 mm Stereo Plug Wiring	20
4.3	Connecting to a Non-Decagon Logger	20
4.4	Pigtail End Wiring	21
5	Communication	23
5.1	SDI-12 Communication	23
6	Understanding Data Outputs	25
6.1	Using Decagon's Em50 series data loggers	25
6.1.1	Up Looking Sensor Outputs	25
6.1.2	Down Looking Sensor Outputs	25
6.2	Using other data loggers	26
7	Installing the SRS	27
7.1	Attaching and Leveling	27
7.2	Cleaning and Maintenance	27

8	Troubleshooting	28
8.1	Data Logger	28
8.2	Sensors	28
8.3	Calibration	28
9	Declaration of Conformity	29

1 Introduction

Thank you for choosing Decagon's Spectral Reflectance Sensor (SRS). We designed the SRS for continuous monitoring of Normalized Difference Vegetation Index (NDVI) and/or the Photochemical Reflectance Index (PRI) of plant canopies. We intend it to be low cost, easily and quickly deployable, and capable of reliable operation over years. Deploy the sensors over plant canopies to record first appearance of green canopy, canopy closure, canopy senescence, light use efficiency, and other variables. Customers can use these measurements to determine light capture, water use, phenology and biomass production. This manual will help you understand the sensor features and how to use this device successfully.

1.1 Customer Support

If you ever need assistance with your sensor, have any questions or feedback, there are several ways to contact us. Decagon has Customer Service Representatives available to speak with you Monday through Friday, between 7am and 5pm Pacific time.

Note: If you purchased your sensor through a distributor, please contact them for assistance.

Email:

support@decagon.com or **sales@decagon.com**

Phone:

509-332-5600

Fax:

509-332-5158

If contacting us by email or fax, please include as part of your message your instrument serial number, your name, address, phone, fax number, and a description of your problem or question.

1.2 About This Manual

Please read these instructions before operating your sensor to ensure that it performs to its full potential.

1.3 Warranty

The sensor has a 30-day satisfaction guarantee and a one-year warranty on parts and labor. Your warranty is automatically validated upon receipt of the instrument.

1.4 Seller's Liability

Seller warrants new equipment of its own manufacture against defective workmanship and materials for a period of one year from the date of receipt of equipment.

Note: We do not consider the results of ordinary wear and tear, neglect, misuse, or accident as defects.

The Seller's liability for defective parts shall in no event exceed the furnishing of replacement parts "freight on board" the factory where originally manufactured. Material and equipment covered hereby which is not manufactured by Seller shall be covered only by the warranty of its manufacturer. Seller shall not be liable to Buyer for loss, damage or injuries to persons (including death), or to property or things of whatsoever kind (including, but not without limitation, loss of anticipated profits), occasioned by or arising out of the installation, operation, use, misuse, nonuse, repair, or replacement of said material and equipment, or out of the use of any method or process for which the same may be employed. The use of this equipment constitutes Buyer's acceptance of the terms set forth in this warranty. There are no understandings, representations, or warranties of any kind, express, implied, statutory or otherwise (including, but without limitation, the implied warranties of merchantability and fitness for a particular purpose), not expressly set forth herein.

2 About SRS

2.1 Overview

The SRS are two-band radiometers that measure either incident or reflected radiation in wavelengths appropriate for calculating the Normalized Difference Vegetation Index (NDVI) or the Photochemical Reflectance Index (PRI). Sensors are manufactured in four different versions: NDVI-hemispherical, NDVI-field stop, PRI-hemispherical and PRI-field stop. The hemispherical versions (Figure 1) are built with Teflon diffusers for making cosine-corrected measurements, and are primarily designed for up looking measurements of incident radiation. The field stop versions (Figure 2) have a field of view restricted to 20° and are designed for pointing downward to measure canopy reflected radiation in NDVI and PRI wavelengths.

The reflected radiation from a vegetated surface is highly variable, depending on the amount and type of vegetation cover. This variability requires a relatively large number of sensors to properly characterize this surface. The field stop and hemispherical versions can both be used to quantify canopy reflected radiation. The correct choice of sensor will depend on the objectives of the study. The hemispherical sensor will do a better job of averaging reflected radiation over a broad area, but if it is not installed normal to the canopy surface it will also average sky, leading to measurement error. The field stop sensor can be aimed at a particular spot or have a particular orientation giving the user more control over what portion of the canopy is being measured. When using the field stop sensor in an off-nadir orientation the user should be careful that the sensor is not pointed above the horizon.

Calculating NDVI or PRI requires knowing both the incoming and reflected radiation. Unlike the reflected radiation, the incoming radiation is spatially uniform above the canopy. So, you only need one up facing radiometer to compute the vegetation indices for many down facing radiometers. The up looking radiometer should be leveled and have a hemispherical field of view.

The SRS is a digital sensor. Its outputs follow the SDI-12 standard. The SRS is best suited for use with Decagon's Em50, Em50R, and Em50G data loggers. However, customers can use the SRS with other loggers, such as those from Campbell Scientific.

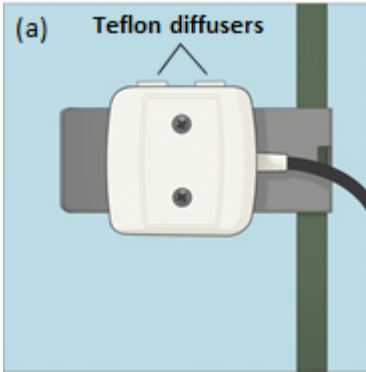


Figure 1: Hemispherical Version

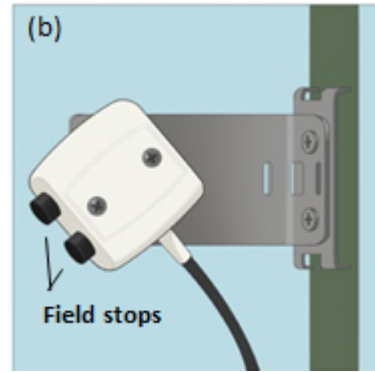


Figure 2: Field Stop Version

2.2 Specifications

Accuracy: 10% or better for spectral irradiance and radiance values

Measurement Time: < 300 ms

NDVI Wavebands: 630 and 800 nm central wavelengths, with 50 and 40 nm full width half maximum band widths

PRI Wavebands: 531 and 571 nm central wavelengths, with 10 nm full width half maximum band widths

Dimensions: 43 x 40 x 27 mm

Power Requirements: 3.6 to 15 V DC, 4 mA (reading, 300 ms) 30 μ A (quiescent)

Operating Temperature: -40 to 50 $^{\circ}$ C

Connector Types: 3.5 mm (stereo) plug or stripped & tinned lead wires (Pigtail)

Cable Length: 5 m standard; custom cable length available upon request.

Other Features:

- SDI-12 digital sensor, compatible with Decagon's EM50 family and CSI loggers
- In-sensor storage of calibration values
- Four versions
 - NDVI-hemispherical
 - NDVI-field stop
 - PRI-hemispherical
 - PRI-field stop
- NDVI or PRI sensors with Teflon cosine correcting heads
- NDVI or PRI sensors with 20 degree field stops sealed with clear acrylic
- NIST traceable calibration to known spectral radiance or irradiance values
- Sensors can be mounted facing up or down, singly or in tandem, leveled or aimed
- Fully sealed from the elements and UV resistant to minimize drift over time

3 Theory

Decagon designed the SRS instruments to measure the NDVI and PRI vegetation indices from plant canopies. We caution users that NDVI and PRI are measurements of electromagnetic radiation reflected from canopy surfaces, and therefore provide indirect or correlative associations with several canopy variables of interest and should not be treated as direct measurements of these variables.

NDVI has a well-established and long history of use in remote sensing research and ecological applications related to canopy structure. PRI, while showing great promise for quantifying canopy physiological function, is far more experimental with new uses and caveats continually being uncovered. While NDVI and PRI can be powerful tools for inferring structure and function of plant canopies, you must take into account their limitations when interpreting the data. Section 3 provides an overview of the theory and discusses some of the uses and limitations of each vegetation index.

3.1 Normalized Difference Vegetation Index (NDVI)

A number of nondestructive methods exist for remotely monitoring and quantifying certain canopy characteristics. Some of those characteristics are: foliar biochemistry and pigment content, leaf area index (LAI, Nguy-Robinson et al., 2012), phenology, and canopy photosynthesis (Ryu et al., 2010). One of the most common nondestructive techniques involves measuring the NDVI. The NDVI is one of a large number of vegetation indices. The principle derives from a well known concept that vegetation reflects light differently in the visible spectrum (400 to 700 nm) compared to the near infrared (> 700 nm).

Green leaves absorb light most strongly in the visible spectrum, but are highly reflective in the near infrared region (Figure 3). Because bare soil, detritus, stems, trunks, branches, and other non-photosynthetic elements show relatively little difference in reflectance between the visible and near infrared, measuring the difference between reflectance in these two bands can be related to the amount

of photosynthetic vegetation in the field of view of a radiometer. See Royo and Dolors (2011) for an extensive introduction to using spectral indices for plant canopy measurements.

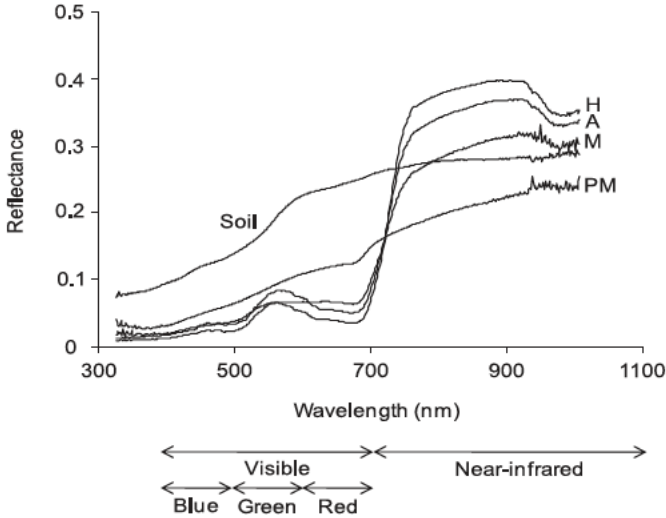


Figure 3: Reflectance spectra for bare soil (Soil) and a healthy wheat crop at various stages of development: heading (H), anthesis (A), milk-grain stage (M), and post maturity (PM). Consider two things about this figure: First, the considerable difference between reflectance spectra from the soil and all stages of plant development. Second, the changes in the visible spectra as the canopy matures and senesces. We reproduced this figure with permission from Royo and Dolors (2011).

Calculate NDVI with equation 1.

$$NDVI = \frac{\rho_{NIR} - \rho_{red}}{\rho_{NIR} + \rho_{red}} \quad (1)$$

Where, ρ_{red} and ρ_{NIR} are percent reflectances in the red and near infrared (NIR). We assume percent reflectance to be the ratio of reflected to incident radiation in the specified waveband. A detailed description of how to calculate reflectances from measured radiation values is provided in equation number 4. NDVI has been shown to

correlate well with green LAI, although the relationship is specific for each crop or natural canopy. For example, Aparicio et al. (2002) studied NDVI versus LAI in more than twenty different durum wheat genotypes in seven experiments over two years and found the relationship shown in Figure 4. Nguy-Robinson (2012) also studied the behavior of NDVI versus LAI in maize and soybean. Their data suggest a similar relationship between the two crops, but not identical. These relationships have been developed for a wide range of crop and natural canopies and we encourage our customers to seek out the best relationship for their application.

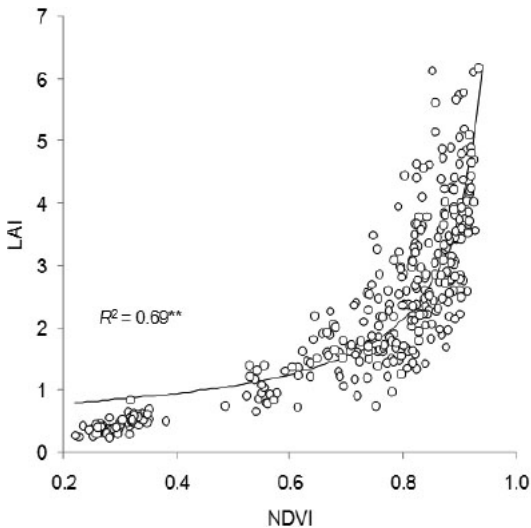


Figure 4: Relationship between leaf area index and NDVI for 20-25 durum wheat genotypes studied over two years in seven different experiments by Aparicio et al. (2002). Values shown were taken at anthesis and milk-grain stage. Used with permission from author.

3.2 Fractional Interception of Photosynthetically Active Radiation

The use of NDVI for determination of leaf area index has limitations. Like many nondestructive techniques (e.g., fisheye and cep-tometer techniques), the measurement of NDVI becomes less and less sensitive as LAI increases above a certain point (Figure 3). Nguy-

Robinson et al. (2012) suggest changes in LAI are difficult to detect when LAI is much greater than $3 \text{ m}^2\text{m}^{-2}$. This should not be surprising considering the spectral measurement being made. NDVI measurements rely on reflected light from leaf surfaces. As the canopy fills and upper leaves begin to cover lower leaves, the leaf area will continue to increase without making a further contribution to reflected radiation. Furthermore, foliar chlorophyll is a very efficient absorber of radiation in red wavelengths so that reflectance from leaves is typically very low in the red region (Figure 3). Therefore, increasing LAI, and thus canopy chlorophyll content does not substantially change red reflectance beyond a certain point. Thus, NDVI has limited predictive ability in canopies with high LAI. For some applications NDVI saturation at high LAI may not be as important as it would appear.

Although the technique may give poor estimates of LAI at high LAI, shaded leaves tend to have much less impact on resource capture compared to sunlit leaves, and therefore contribute proportionally less to canopy productivity. As a general modeling parameter, an estimate of sunlit leaves may be adequate for estimating photosynthesis and biomass accumulation (i.e., carbon uptake) for some applications. Monteith (1977) proposed the now well-known relationship between biomass accumulation and radiation capture seen in equation 2.

$$A_{n, \text{canopy}} = \epsilon f_s S_t \quad (2)$$

In equation 2, $A_{n, \text{canopy}}$ is the biomass accumulation or carbon assimilation and ϵ is a conversion efficiency often referred to as light use efficiency (LUE). The LUE depends on a variety of factors such as photosynthetic acclimation, physiological stress level, and plant species. f_s is the fractional interception of radiation by the canopy, and S_t is the total incident radiation. The relationship between NDVI and LAI in Nguy-Robinson et al. (2012) and the relation between fractional interception and LAI (Campbell and Norman, 1998) show that NDVI and fractional interception are approximately related linearly (Figure 5). NDVI can provide a good estimate of the fractional interception by green leaves in a canopy; a value that is critical for carbon assimilation models.

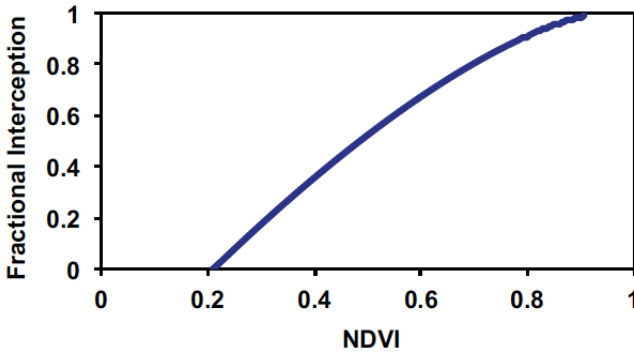


Figure 5: Relationship between fractional canopy interception and NDVI, where NDVI is converted to LAI using Nguy-Robinson et al. (2012). Campbell and Norman (1998) give the relationship between LAI and fractional interception.

3.3 Canopy Phenology

Like all spectral measurements, NDVI is an indirect measurement. Over the years, researchers have correlated parameters of interest, like LAI and f_s , to measurements made at 630 nm and 800 nm. Researchers have estimated other variables using NDVI besides these relationships. Two of these variables are the focus of Ryu et al. (2010), who used a simple two-band LED-based sensor, similar to the SRS-NDVI, to measure canopy phenology and associated changes in photosynthesis in an annual grassland over a four year period. Ryu et al (2010). show an exponential relationship between NDVI and canopy photosynthesis, but found that the LAI of grassland never increases above $2.5 \text{ m}^2 \text{ m}^{-2}$. Ecosystem phenology can also be tracked in the time series data from their NDVI sensor with errors on the order of a few days. It should be noted that they filtered their data by limiting NDVI measurements to a particular sun elevation angle (e.g., sampling under identical sun zenith and azimuth angles from day to day).

3.4 Photochemical Reflectance Index (PRI)

As described above, the NDVI is primarily useful as a proxy for canopy structural variables. Although structural properties are critical, sometimes it is useful to have information about canopy functional properties. For example, estimating the gross primary productivity (GPP) of ecosystems is critical for modeling the global carbon balance. The simple model presented in Equation 2 can be used to predict GPP from three variables: incident light (S_t), intercepted light (f_s), and light use efficiency (ϵ). S_t can generally be estimated depending on geographic location and time of day or measured with a PAR sensor or pyranometer. Considering the near linear relationship between NDVI and fractional interception noted above, a simple two-band spectral reflectance sensor like the SRS-NDVI can provide an estimate of f_s . The light use efficiency term (ϵ) remains to be quantified in order to make accurate predictions of GPP.

Gamon et al. (1990, 1992) proposed a dual band vegetation index (similar to the NDVI) to predict ϵ . The foundation of the measurement is based on the absorbance of xanthophyll pigments at 531 nm that correlates with LUE in many plant species (Gamon et al., 1997). This ratio is called the Photochemical Reflectance Index (PRI) and is calculated with Equation 3.

$$PRI = \frac{\rho_{531} - \rho_{570}}{\rho_{531} + \rho_{570}} \quad (3)$$

Where, ρ_{531} and ρ_{570} are percent reflectances at 531 and 570 nm, respectively. When combined, you can use NDVI and PRI to predict biomass accumulation or GPP of an ecosystem without the expense and work of some of the other approaches (Gamon et al., 2001). Because of the low cost, light weight, small footprint and low power use of the sensors, they can be deployed very quickly, over long periods of time, or in a spatially distributed network to quantify spatiotemporal variations in canopy productivity (Garrity et al., 2010).

In addition to LUE, the PRI has also been shown to correlate with numerous other physiological variables associated with plant photosynthetic performance from the leaf to the ecosystem level (Gamon et al., 1992, 1997, 2001). Xanthophylls absorb radiation at 531 nm and

will absorb more radiation as a consequence of saturation of chlorophyll centers. A normalized difference of reflectance at 570 nm that remains unchanged despite changes in light saturation to 531 nm will indicate the level of xanthophyll absorbance and the efficiency of plant light use. Because increased xanthophyll absorbance is not solely correlated with LUE, researchers have investigated many other relationships too.

Numerous studies correlate PRI to various ecophysiological variables including the epoxidation state of xanthophyll, maximum photochemical efficiency of photosystem II, effective quantum yield, maximum photosynthesis rate, electron transport under saturating light, non-photochemical quenching, and chlorophyll to carotenoid content ratio (Sims & Gamon, 2002; Garrity et al., 2011; Garbulsky et al., 2011; Porcar-Castell et al., 2012). Garbulsky et al. (2011) and Porcar-Castell et al. (2012) provide excellent overviews of what has been done with PRI including analyses of PRI correlations with several of these variables at the leaf, canopy, and ecosystem levels. We encourage our customers to use these references as a starting resource.

3.5 Sun-Sensor-Surface Geometry Considerations

Spectral reflectance measurements are inherently variable due to radiation source, reflecting surface, and sun-sensor-surface geometry. Hence, it is not uncommon for a time series of NDVI or PRI to contain high amounts of variability. Consider changes in daily NDVI measured at four-day intervals in a subalpine meadow. (Figure 6) Figure 6 shows the control treatment green-up under drought conditions. The well-watered treatment in Figure 7 includes the same time period but has already undergone initial green-up.

There are three things to notice about these data. First, canopy green-up is clearly visible in the time series of the control (upper graph) treatment. Second, the track of daily NDVI is generally concave, which indicates that sampling across a consistent sun angle (e.g. 60° elevation angle (Ryu et al., 2012)) or around solar noon is advisable when summarizing an entire day to a single value. If comparing

measurements acquired under different sun-sensor-surface configurations, it is necessary to first calculate a bidirectional reflectance distribution function (BRDF). Once you have empirically derived a BRDF model from the measurements and canopy-specific parameters, you can use it to reduce variations that arise from changes in sun-sensor-surface geometry across diurnal time series. For additional details on BRDF normalization of vegetation index time series, see Hilker et al. (2008).

Sometimes NDVI values will exhibit erratic behavior due to environmental conditions (see Day 178 on both graphs). Data filtering (e.g., visual inspection for short time series or automated despiking algorithms for longer time series) may be required to remove spurious data points.

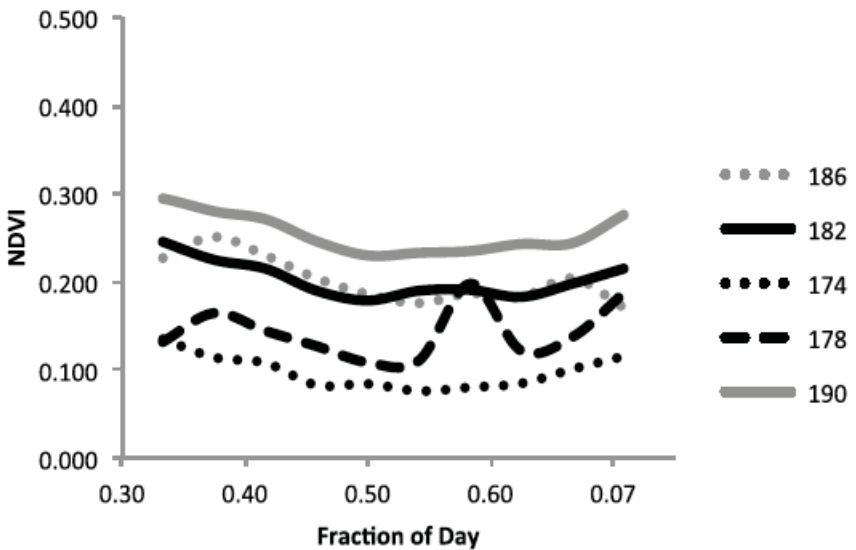


Figure 6: Daily variation in NDVI measurements 1 m above a sub-alpine meadow

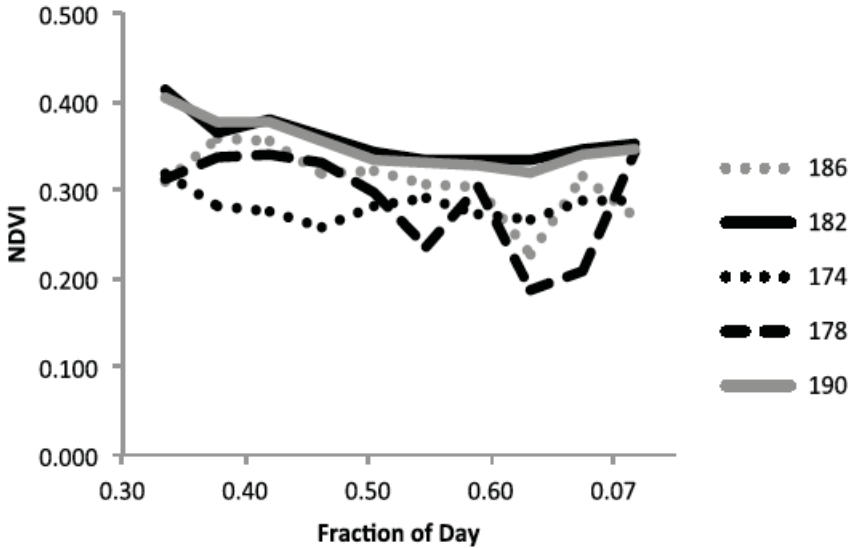


Figure 7: Another daily variation in NDVI measurements 1 m above a sub-alpine meadow

3.6 Calculating Percent Reflectance from Paired Up and Down Looking Sensors

Equation 1 shows that NDVI is the ratio of the difference to the sum of NIR and red reflectances. Each reflectance is the ratio of upwelling (down looking sensor) to incident (up looking sensor) radiant flux in each of the wave bands. Calculating this ratio is only possible when measurements of downwelling and upwelling radiation are collected simultaneously under the same ambient conditions. Combining measurements made with sensors located long distances apart is typically not recommended because atmospheric conditions (e.g., cloud cover, aerosols) can be highly variable in space. Reasonable distances between up looking and down looking sensors will depend on the typical radiation environment of a given location.

It is also important to arrange paired up looking and down looking sensors to collect data at the same time, which will account for

temporal variability in radiation conditions. In cases where multiple down looking sensors have been deployed within close proximity to each other, it is only necessary to have one up looking sensor. The measurements from the single up looking sensor can be combined with the measurements from each of the down looking sensors to calculate reflectances

In the event that up looking measurements are not available, rearrangement of the vegetation index equations allows for a rough approximation of the measurements. The following derivation is for NDVI, but similar equations apply to the PRI. If R_n is the reflected NIR radiation from the canopy, R_r is the reflected red radiation, I_n is the incident NIR, and I_r is the incident red, then

$$NDVI = \frac{R_n/I_n - R_r/I_r}{R_n/I_n + R_r/I_r} = \frac{(I_r/I_n)R_n - R_r}{(I_r/I_n)R_n + R_r} = \frac{\alpha R_n - R_r}{\alpha R_n + R_r} \quad (4)$$

Where $\alpha = I_r/I_n$, equation 4 allows the computation of NDVI from just the down facing measurements if you know the ratio of red to NIR spectral irradiance, α . Although not extensively tested, we have found that this ratio ($\alpha = 1.86$ for NDVI bands) can be used as a rough approximation during midday under relatively clear sky conditions. However, we caution that direct measurements of downwelling radiation is more accurate by accounting for any fluctuations in α that occur with changes in atmospheric conditions or across large variations in sun elevation angle.

In the event that you do not want to use the default α value or measurements from an up facing sensor are not available, it is possible to use a spectralon panel or similar reflectance standard with a field stop SRS to measure incident irradiance. To measure incident irradiance with a down facing sensor, place a reflectance standard within the field of view of the field stop sensor, making sure that the reflectance panel is level, uniformly illuminated and that the field of view of the sensor is fully within the area of the reflectance panel. Measurements obtained from field stop sensors pointed at the reflectance panel must be multiplied by π to convert radiance values to irradiance values. Irradiance values can then be used in Equation 4 or to calculate α directly.

References

- Aparicio, N., Villegas, D., Casadesus, J., Araus, J.L., and Royo, C., (2000). Spectral vegetation indices as nondestructive tools for determining durum wheat yield. *Agronomy Journal*, 92: 83-91.
- Aparicio, N.; Villegas, D.; Araus, J.L.; Casadess, J.; Royo, C., (2002). Relationship between growth traits and spectral reflectance indices in durum wheat. *Crop Science*, 42: 1547-1555.
- Campbell, G.S. and Norman, J.M., (1998). An Introduction to Environmental Biophysics. Springer-Verlag. New York.
- Gamon, J.A., Field, C.B., Bilger, W., Bjorkman, O., Fredeen, A.L., Peuelas, J., (1990). Remote sensing of the xanthophylls cycle and chlorophyll fluorescence in sunflower leaves and canopies. *Oecologia*, 85: 1-7.
- Gamon, J.A., Peuelas, J., Field, C.B., (1992). A narrow-waveband spectral index that tracks diurnal changes in photosynthetic efficiency. *Remote Sensing of Environment*, 41: 35-44.
- Gamon, J. A., Serrano, L., Surfus, J. S., (1997). The photochemical reflectance index: an optical indicator of photosynthetic radiation use efficiency across species, functional types, and nutrient levels. *Oecologia*, 112: 492-501.
- Gamon, J. A., Field, C. B., Fredeen, A. L., Thayer, S., (2001). Assessing photosynthetic downregulation in sunflower stands with an optically based model. *Photosynthesis Research*, 67: 113-125.
- Garbulsky, M.F., Peuelas, J., Gamon, J., Inoue, Y., Filella, Y. (2011). The photochemical reflectance index (PRI) and the remote sensing of leaf, canopy and ecosystem radiation use efficiencies: A review and meta-analysis. *Remote Sensing of the Environment*, 115: 281-297.
- Garrity, S.R., Vierling, L.A., Bickford, K., (2010). A simple filtered photodiode instrument for continuous measurement of narrowband

NDVI and PRI over vegetated canopies. *Agricultural & Forest Meteorology*, 150: 489-496.

Garrity, S. R., Eitel, J. U. H., Vierling, L. A., (2011). Disentangling the relationships between plant pigments and the photochemical reflectance index reveals a new approach for remote estimation of carotenoid content. *Remote Sensing of Environment*, 115: 628-635.

Hilker, T., Coops, N. C., Hall, F. G., Black, T. A., Wulder, M. A., Nesic, Z., Krishnan, P., (2008). Separating physiologically and directionally induced changes in PRI using BRDF models. *Remote Sensing of Environment*, 112: 2777-2788.

Monteith, J.L., (1977). Climate and the efficiency of crop production in Britain. *Philosophical Transactions Royal Society of London B*, 281: 277-294.

Nguy-Robertson, A. Gitelson, A., Peng, Y., Via, A., Arkebauer, T., and Rundquist, D., (2012). Green leaf area index estimation in maize and soybean: Combining vegetation indices to achieve maximal sensitivity. *Agronomy Journal*, 104: 1336-1347.

Porcar-Castell, A., Garcia-Plazaola, J. I., Nichol, C. J., Kolari, P., Olascoaga, B., Kuusinen, N., Fernandez-Marn, B., Pulkkinen, M., Juurola, E., Nikinmaa, E., (2012). Physiology of the seasonal relationship between the photochemical reflectance index and photosynthetic light use efficiency. *Oecologia*, 170: 313-323.

Royo, C. and Villegas, D., (2011). Field Measurements of Canopy Spectra for Biomass Assessment of Small-Grain Cereals, Biomass - Detection, Production and Usage, Darko Matovic (Ed.), ISBN: 978-953-307-492-4, InTech, Available from: <http://www.intechopen.com/books/biomass-detection-production-and-usage/field-measurements-of-canopy-spectra-for-biomass-assessment-of-small-grain-cereals>.

Ryu, Y., Baldocchi, D.D., Verfaillie, J., Ma, S., Falk, M., Ruiz-Mercado, I., Hehn, T., Sonnentag, O., (2012). Testing the performance of a novel spectral reflectance sensor, built with light emit-

ting diodes (LEDs), to monitor ecosystem metabolism, structure and function. *Agricultural & Forest Meteorology*, 150: 1597-1606.

Sims, D. A., Gamon, J. A., (2002). Relationships between leaf pigment content and spectral reflectance across a wide range of species, leaf structures and developmental stages. *Remote Sensing of Environment*, 81: 337-354.

4 Connecting the SRS

4.1 Connecting to Decagon Data Logger

The SRS is most easily used with Decagon's Em50, Em50R and Em50G loggers (firmware version 2.13 or later). SRS sensors can also be used with other SDI-12 enabled data loggers, such as those from Campbell Scientific, Inc. The SRS requires an excitation voltage in the range of 3.6 to 15 volts.

To download data to your computer from an Em50 series logger, you will need to install ECH₂O Utility or DataTrac 3 on your computer. The following software supports the SRS sensor:

Em50 Firmware version 2.14 or greater

ECH₂O Utility 1.68 or greater

DataTrac 3.8 or greater

ProCheck 1.51 or greater

Note: Please check your software version to ensure it will support the SRS.

To update your software to the latest versions, please visit Decagon's support site at <http://www.decagon.com/support/>.

To use the SRS with your Em50 series data logger, simply plug the stereo plug into one of the five ports on the data logger and use either ECH₂O Utility, or DataTrac 3 software (see respective manuals) to configure that port for the SRS and set the measurement interval.

The highest logging frequency for the Em50 and Em50R data loggers is one minute and for the Em50G logger it is five minutes. When you set the logging interval to greater than one minute on any of the Em50 series loggers, reported readings are automatically averaged using data sampled from the sensor at one minute intervals. Users need to be cautious when choosing a sampling interval with SRS sensors connected to an Em50 series logger, so that the averaging feature does not result in erroneous measurement. For example, if

you desire only one reading per day and you select 24 hours as the measurement interval, then each 24 hour reading will be an average of values recorded over the previous 1,440 minutes, including periods during the night. To avoid such errors, we recommend you log data from the SRS sensors more frequently, even if you are not using all logged data.

If customers require logging intervals shorter than one minute, then they must use a Campbell Scientific or similar logger capable of recording data at the desired frequency.

4.2 3.5 mm Stereo Plug Wiring

The SRS for Decagon loggers ships with a 3.5 mm stereo plug connector. The stereo plug allows for rapid connection directly to Decagon's Em50 and Em50G data loggers. Figure 8 shows the wiring configuration for this connector.



Figure 8: 3.5 mm Stereo Plug Wiring

4.3 Connecting to a Non-Decagon Logger

Customers may purchase the SRS for use with non-Decagon data loggers. These sensors typically come configured with stripped and tinned (pigtail) lead wires for use with SDI BUS terminals. Refer to your particular logger manual for details on wiring. Our integrator's guide gives detailed instructions on connecting the SRS to non-Decagon loggers. Please visit www.decagon.com/support for the complete integrator's guide.

4.4 Pigtail End Wiring



Figure 9: Pigtail End Wiring

SRS sensors with the stripped and tinned cable option can be made with custom cable lengths (up to 305 meters) on a per meter fee basis. This option gets around the need for splicing wire (a possible failure point). Connect the wires to the data logger as Figure 10 shows. Connect the supply wire (white) to the excitation, the digital out wire (red) to a digital input, and the bare ground wire to ground.

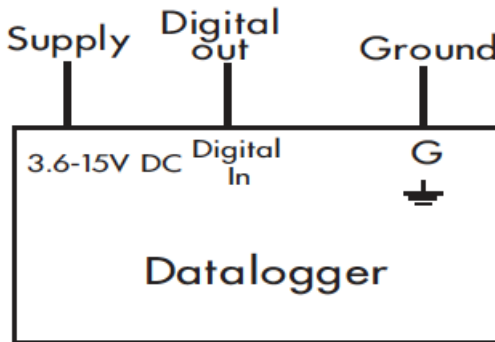


Figure 10: Pigtail End Wiring to Data Logger

Note: The acceptable range of excitation voltages is from 3.6 to 15 VDC. If you wish to read the SRS with the Campbell Scientific Data Loggers, you will need to power the sensors off of a 12 V or switched 12 V port.

If your SRS is equipped with the standard 3.5 mm plug, and you wish to connect it to a non-Decagon data logger, you have two op-

tions. First, you can clip off the plug on the sensor cable, strip and tin the wires, and wire it directly into the data logger. This has the advantage of creating a direct connection with no chance of the sensor becoming unplugged; however, it then cannot be easily used in the future with a Decagon data logger. The other option is to obtain an adapter cable from Decagon. The 3-wire sensor adapter cable has a connector for the sensor jack on one end, and three wires on the other end for connection to a data logger (this is referred to as a “pigtail adapter,” Figure 10). Both the stripped and tinned adapter cable wires have the same termination as seen above; the white wire is excitation, red is data output, and the bare wire is ground.

Note: Be extra careful to secure your stereo to pigtail adapter connections to ensure that sensors do not become disconnected during use.

5 Communication

The SRS communicates using SDI-12 protocol. This chapter discusses the specifics of SDI-12 Communication. For more information, please visit www.decagon.com/support for an integrator's guide that gives more detailed explanations and instructions.

5.1 SDI-12 Communication

The SRS communicates using the SDI-12 protocol, a three-wire interface where all sensors are powered (white wire), grounded (bare wire) and communicate (red wire) on shared wires (for more info, go to www.sdi-12.org). There are some positive and negative elements of this protocol. On the positive side, multiple sensors can be connected to the same 12 V supply and communication port on the data logger. This simplifies wiring because no multiplexer is necessary. On the negative side, one sensor problem can bring down the entire array (through a short circuit, etc.). To mitigate this problem, we recommend the user make an independent junction box with wire harnesses where all sensor wires are connected to binding posts so you can disconnect sensors if a problem arises. A single three-wire bundle can be run from the junction box to the data logger.

The SDI-12 protocol requires that each sensor have a unique address. The SRS comes from the factory with an SDI-12 address of 0. To add more than one SDI-12 sensor to a system, the sensor address must change. Address options include 0-9, A-Z, a-z. There are two ways to set the SDI-12 sensor address. The best and easiest is to use Decagon's ProCheck (if the option is not available on your ProCheck, please upgrade to the latest version of firmware). Access SDI-12 addressing in the "CONFIG" menu by selecting "SDI-12 Address" and pressing Enter. To change the SDI-12 address, press the up and down arrows until you see the desired address and push Enter. SDI-12 communication allows many parameters to be communicated at once, so you can also see things like the sensor model, SDI-12 version, etc.

Campbell Scientific data loggers, like the CR10X, CR1000, CR3000,

among others, also support SDI-12 Communication. Direct SDI-12 communication is supported in the “Terminal Emulator” mode under the “Tools” menu on the “Connect” screen. Detailed information on setting the address using CSI data loggers can be found on our website at <http://www.decagon.com/support/downloads/>.

The sensor can be powered using any voltage from 3.6 to 15 V DC. The SDI-12 protocol allows the sensors to be continuously powered, so the power (white wire) can be connected to a continuous 12 VDC source. However, the sensor can also be used with a switched 12 V source. This can help reduce power use (although the SRS uses very little power, 0.03 mA quiescent) and will allow the sensor array to be reset if a problem arises.

Reading the SRS in SDI-12 mode using a CSI data logger requires a function call. An example program from Edlog and CRBasic can be found in the software section of <http://www.decagon.com/support/>.

6 Understanding Data Outputs

6.1 Using Decagon's Em50 series data loggers

Each SRS sensor generates multiple outputs when connected to Decagon's Em50 data logger. The exact outputs will in part depend on how many and what type of SRS sensors are attached to the data logger. All SRS sensors are equipped with an internal tilt sensor. The orientation of the SRS, and therefore the tilt sensor, will determine the output from each sensor.

6.1.1 Up Looking Sensor Outputs

For any hemispherical sensor oriented in the up looking position, outputs will include the calibrated spectral irradiance ($\text{W m}^{-2} \text{nm}^{-1}$) and α , where α is the ratio of 630 nm to 800 nm for NDVI sensors and 570 nm to 532 nm for PRI sensors. See Equation 4 for further details on α .

6.1.2 Down Looking Sensor Outputs

When hemispherical or field stop sensors are mounted in a down-looking orientation, outputs include the calibrated spectral radiance ($\text{W m}^{-2} \text{nm}^{-1} \text{sr}^{-1}$) of each band and either NDVI or PRI. If both up looking and down looking sensors of the same variety (e.g., up looking hemispherical NDVI and down looking field stop NDVI) are connected to the same data logger then α from the up looking sensor is combined with the spectral radiance values from the down looking sensor to calculate the vegetation index, using Equation 4. In the event that only down looking sensors are connected to a data logger, then either the default or the user-specified static α value is used to calculate the vegetation index. Based on observations collected near Pullman, WA ($46^{\circ}45'0''\text{N}$, $117^{\circ}09'6''\text{W}$), default α values have been set to 0.98 and 1.86 for PRI and NDVI, respectively. Note that actual values of α will change depending on atmospheric conditions and sun angle, so users are encouraged to measure α with an up looking hemispherical sensor. In the event that nearby up looking and

down looking sensors are connected to different data loggers, you can export tabular data as Excel files and manually combine α from the up looking sensor with the spectral radiance values from the down looking sensor to calculate NDVI or PRI.

6.2 Using other data loggers

When connected to non-Decagon data loggers (e.g., Campbell Scientific) sensors will output the calibrated spectral irradiance or radiance from each band and an orientation value from the tilt sensor. Spectral irradiance and radiance are output as radiant fluxes (in $\text{W m}^{-2} \text{nm}^{-1}$ or $\text{W m}^{-2} \text{nm}^{-1} \text{sr}^{-1}$) for the shorter and then the longer wavelength sensor. Tilt sensor readings are output as a single value between 0 and 2, with 0 indicating an indeterminate orientation, 1 indicating a down facing orientation, and 2 indicating an up facing orientation. Additional information about using the SRS with non-Decagon data loggers can be accessed at www.decagon.com/srs. For additional information about connecting your SRS to non-Decagon data loggers, see Section 4.3.

7 Installing the SRS

7.1 Attaching and Leveling

The SRS comes with a variety of mounting hardware, allowing it to be mounted on posts, rebar, poles, tripods, etc. The mounting hardware allows for vertical adjustment and orientation on the pole and allows for sensor tilt. Up-facing sensors have Teflon diffusers and measure radiation from the entire upper hemisphere. The sensor therefore needs to be leveled and mounted in a location where it will not be shaded and has an unobstructed view of the sky.

For down-facing sensors, the SRS can be mounted any distance from the canopy, but it is important to keep in mind that the influence of individual plants on the reading increases as the sensor gets closer to the canopy.

You may use hemispherical down facing sensors, but make sure to mount them facing directly down so they are not “seeing” sky. The influence of the pole and sky can be avoided by using field stop radiometers. These will average over just the area within the 20° field of view where you aimed them. Assure that the area they see is representative and carefully choose the view elevation and azimuth. When the view angle is directly away from the sun the sensor sees mostly sunlit leaves. If it points perpendicular to the sun rays the sensor will see an increased fraction of shadow. Field stop sensors are intended for measuring canopy-reflected radiation and should not be mounted in an up facing orientation.

7.2 Cleaning and Maintenance

Optical surfaces need to be kept clean and free from dust, debris and deposits. Clean surfaces with water and a soft cloth as necessary. Return the radiometer to the factory for recalibration after approximately one year of outdoor exposure. See section 7.3 for more details on calibration.

8 Troubleshooting

Any problem with the SRS will most likely manifest as failed communication or erroneous readings. Before contacting Decagon about the sensor, please check these troubleshooting steps.

8.1 Data Logger

1. Check to make sure the connections to the data logger are both correct and secure.
2. Ensure that your data logger batteries are not dead or loose.
3. Check the configuration of your data logger in ECH₂O Utility or DataTrac 3 to make sure you have selected the correct SRS version (NDVI or PRI).
4. If using Decagon loggers make sure that you are using the correct versions of logger firmware and software.

8.2 Sensors

1. Ensure that you install the sensors according to the “Installation” section of this manual.
2. Check sensor cables for nicks or cuts that could cause a malfunction.

8.3 Calibration

Decagon Devices Inc. factory calibrates the Spectral Reflectance Sensor against a NIST traceable light source. Details about your sensor calibration are available upon request. We have a recalibration service available and recommend that you send in your SRS sensors for recalibration every one to two years. You will need a Return Material Authorization (RMA) form to send your sensor in for recalibration. Call or email Decagon at 509-332-5600 or support@decagon.com to arrange for a RMA, or to obtain your sensor calibration information.

9 Declaration of Conformity

Application of Council Directive:	89/336/EE6
Standards to which conformity is declared:	EN61326 : 1998 and EN500082 : 1998
Manufacturer's Name:	Decagon Devices, Inc 2365 NE Hopkins Ct. Pullman, WA 99163 USA
Type of Equipment:	Spectral Reflectance Sensor
Model Number:	SRS
Year of First Manufacture:	2013

This is to certify that the SRS Spectral Reflectance Sensor, manufactured by Decagon Devices, Inc., a corporation based in Pullman, Washington, USA meets or exceeds the standards for CE compliance as per the Council Directives noted above. All instruments are built at the factory at Decagon and pertinent testing documentation is freely available for verification.

Index

- Calibration, 28
- CE Compliance, 29
- Cleaning, 27
- Connecting Sensors
 - Non-Decagon Logger, 20
- Connecting the Sensors, 19
- Contact Information, 1
- Customer Support, 1

- Declaration of Conformity, 29

- Email, 1

- Fax, ii
- Fractional Interception, 8

- Installation, 27

- Leaf Area Index(LAI), 6

- Measurement Angle, 12

- NDVI, 6

- Phenology, 10
- Phone, ii
- Photochemical Reflectance Index,
 - 1
- Photosynthesis, 10
- Pigtail End Wiring, 21

- SDI-12 Communication, 23
- Seller's Liability, 2
- Specifications, 4
- Stereo Wiring 3.5 mm, 20

- Troubleshooting, 28

- Warranty, 2