



METER

TEROS 31 INTEGRATOR GUIDE

SENSOR DESCRIPTION

The TEROS 31 Soil Water Potential and Temperature sensor is a precision tensiometer that measures water potential in the critical range (-85 kPa to $+50$ kPa) for water movement, critical range for plant response, and laboratory lysimeter experiments. With a ceramic diameter of only 5 mm, the TEROS 31 has all the advantages of small dimensions: little soil disturbance, selective pick-up, and fast response. Tensiometers will require periodic refilling when measurements go beyond the measuring range of the sensor.

For a more detailed description of how this sensor makes measurements, refer to the [TEROS 31 User Manual](#).

APPLICATIONS

- Soil–water tension measurement
- Soil–water storage measurement
- Irrigation management
- Soil temperature measurement
- In-situ retention curves

ADVANTAGES

- Plug-and-play tensiometer
- Digital sensor communicates multiple measurements over a serial interface
- Low-input voltage requirements
- Low-power design supports battery-operated data loggers
- Supports SDI-12 or DDI serial communications protocols
- Modbus® RTU or tensioLINK® serial communications protocol supported

PURPOSE OF THIS GUIDE

METER provides the information in this integrator guide to help TEROS 31 customers establish communication between these sensors and their data acquisition equipment or field data loggers. Customers using data loggers that support SDI-12 sensor communications should consult the data logger user manual. METER sensors are fully integrated into the METER system of plug-and-play sensors, cellular-enabled data loggers, and data analysis software.

COMPATIBLE FIRMWARE VERSIONS

This guide is compatible with firmware versions 2.5.0 or newer.

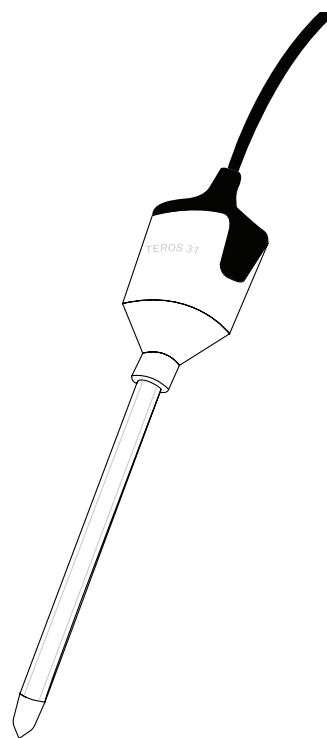


Figure 1 TEROS 31 sensor

SPECIFICATIONS

MEASUREMENT SPECIFICATIONS

Water Potential	
Range	–85 to +50 kPa (up to –400 kPa during boiling retardation)
Resolution	±0.0012 kPa
Accuracy	±0.15 kPa
Temperature	
Range	–30 to +60°C
Resolution	±0.01 °C
Accuracy	±0.3 °C between +5°C to 35°C (±1.5 °C outside the range)
NOTE: If the sensor unit is not buried, measured temperature may diverge from soil temperature.	

COMMUNICATION SPECIFICATIONS

Output
DDI Serial SDI-12 communication protocol tensioLINK® communication protocol Modbus® RTU communication protocol
Data Logger Compatibility
METER ZL6 and EM60 data loggers or any data acquisition system capable of 3.6- to 28.0-VDC excitation and SDI-12, Modbus RTU, or tensioLINK communication.
BARO Module
The BARO Module is an atmospheric pressure sensor that can use different connectors to connect directly between a TEROs 31 and a non-METER data logger. The logger obtains a barometric compensated analog matrix potential signal. The BARO Module can be used for varied logger communications: SDI-12, Modbus, tensioLINK, analog voltage signal.

PHYSICAL SPECIFICATIONS

Dimensions	
Width	23.5 mm (0.93 in)
Depth	17.5 mm (0.69 in)
Height	49.0 mm (1.93 in)
Shaft Diameter	
5 mm (0.19 in)	
Shaft Length	
2, 5, 7, 10, 15, or 20 cm	

Operating Temperature Range	
Minimum	0 °C
Maximum	50 °C
Materials	
Ceramic	Al ₂ O ₃ , bubble point 500 kPa
Shaft	PMMA
Sensor Unit	PMMA and TPE
IP Rating	IP 67
Cable Length	
1.5 m	
Cable Diameter	
<3.0 mm (<0.12 in)	
Connector Types	
4-pin stereo plug connector	
Stereo Plug Connector Diameter	
3.50 mm	
Conductor Gauge	
31 AWG drain wire	

ELECTRICAL AND TIMING CHARACTERISTICS

Supply Voltage (VCC to GND)	
Minimum	3.6 V
Typical	12.0 V
Maximum	28.0 V
Digital Input Voltage (logic high)	
Minimum	1.6 V
Typical	3.3 V
Maximum	5.0 V
Digital Input Voltage (logic low)	
Minimum	–0.3 V
Typical	0.0 V
Maximum	0.9 V
Digital Output Voltage (logic high)	
Minimum	NA
Typical	3.6 V
Maximum	NA

Power Line Slew Rate		Power Up Time (SDI-12)	
Minimum	1.0 V/ms	Minimum	125 ms
Typical	NA	Typical	130 ms
Maximum	NA	Maximum	150 ms
Current Drain (during measurement)		Power Up Time (SDI-12, DDI Serial disabled)	
Minimum	18.0 mA	Minimum	125 ms
Typical	25.0 mA	Typical	130 ms
Maximum	30.0 mA	Maximum	150 ms
Current Drain (while asleep)		Measurement Duration	
Minimum	0.03 mA	Minimum	60 ms
Typical	0.05 mA	Typical	65 ms
Maximum	0.09 mA	Maximum	70 ms
Power Up Time (DDI Serial)		COMPLIANCE	
Minimum	125 ms	EM ISO/IEC 17050:2010 (CE Mark)  CE	
Typical	130 ms		
Maximum	150 ms		

EQUIVALENT CIRCUIT AND CONNECTION TYPES

Refer to [Figure 2](#) and [Figure 3](#) to connect the TEROS 31 to a data logger. [Figure 2](#) provides a low-impedance variant of the recommended SDI-12 specification.

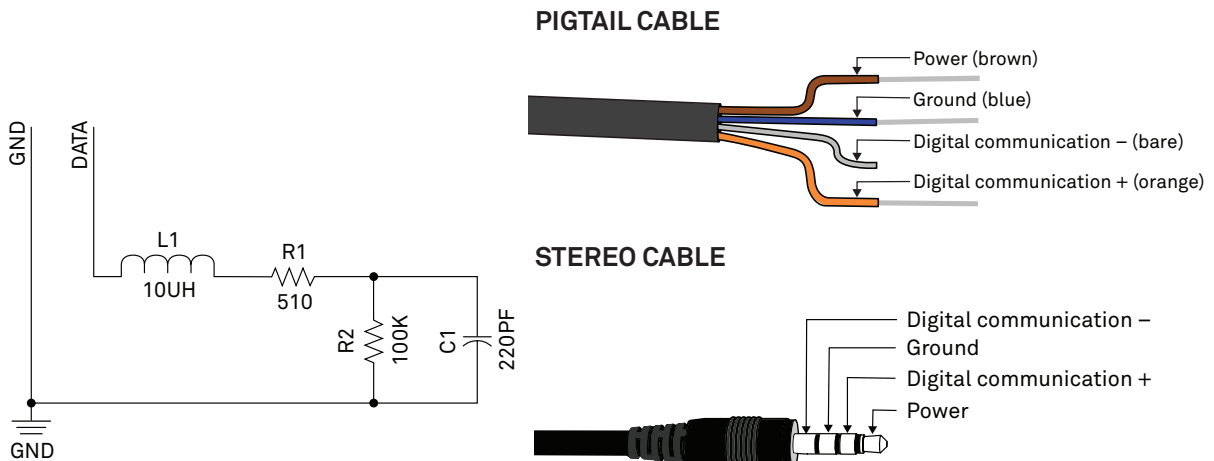


Figure 2 Equivalent circuit diagram

Figure 3 Connection types

PRECAUTIONS

METER sensors are built to the highest standards, but misuse, improper protection, or improper installation may damage the sensor and possibly void the warranty. Before integrating sensors into a sensor network, follow the recommended installation instructions and implement safeguards to protect the sensor from damaging interference.

SURGE CONDITIONS

Sensors have built-in circuitry that protects them against common surge conditions. Installations in lightning-prone areas, however, require special precautions, especially when sensors are connected to a well-grounded third-party logger.

Read the application note [Lightning surge and grounding practices](https://meter.ly/lightning-surge-grounding-practices) on the METER website for more information (meter.ly/lightning-surge-grounding-practices).

POWER AND GROUNDING

Ensure there is sufficient power to simultaneously support the maximum sensor current drain for all the sensors on the bus. The sensor protection circuitry may be insufficient if the data logger is improperly powered or grounded. Refer to the data logger installation instructions. Improper grounding may affect the sensor output as well as sensor performance.

Read the application note [Lightning surge and grounding practices](https://meter.ly/lightning-surge-grounding-practices) on the METER website for more information (meter.ly/lightning-surge-grounding-practices).

CABLES

Improperly protected cables can lead to severed cables or disconnected sensors. Cabling issues can be caused by many factors, including rodent damage, driving over sensor cables, tripping over the cable, not leaving enough cable slack during installation, or poor sensor wiring connections. To relieve strain on the connections and prevent loose cabling from being inadvertently snagged, gather and secure the cable travelling between the Teros 31 and the data acquisition device to the mounting mast in one or more places. Install cables in conduit or plastic cladding when near the ground to avoid rodent damage. Tie excess cable to the data logger mast to ensure cable weight does not cause sensor to unplug.

SENSOR COMMUNICATIONS

METER digital sensors feature a serial interface with shared receive and transmit signals for communicating sensor measurements on the data wire ([Figure 3](#)). The sensor supports four different protocols: SDI-12 and DDI serial one-wire, as well as tensioLINK and Modbus over RS-485 two-wire. The sensor automatically detects the interface and protocol which is being used. Each protocol has implementation advantages and challenges. Please contact METER [Customer Support](#) if the protocol choice for the desired application is not obvious.

SDI-12 INTRODUCTION

SDI-12 is a standards-based protocol for interfacing sensors to data loggers and data acquisition equipment. Multiple sensors with unique addresses can share a common 3-wire bus (power, ground, and data). Two-way communication between the sensor and logger is possible by sharing the data line for transmit and receive as defined by the standard. Sensor measurements are triggered by protocol command. The SDI-12 protocol requires a unique alphanumeric sensor address for each sensor on the bus so that a data logger can send commands to and receive readings from specific sensors.

Download the [SDI-12 Specification v1.3](#) to learn more about the SDI-12 protocol.

DDI SERIAL INTRODUCTION

The DDI serial protocol is the method used by the METER data loggers for collecting data from the sensor. This protocol uses the data line configured to transmit data from the sensor to the receiver only (simplex). Typically, the receive side is a microprocessor UART or a general-purpose I/O pin using a bitbang method to receive data. Sensor measurements are triggered by applying power to the sensor.

RS-485 INTRODUCTION

RS-485 is a robust physical bus connection to connect multiple devices to one bus. It is capable of using very long cable distances under harsh environments. Teros 31 uses a 2-wire, half-duplex implementation of RS-485. Two wires are used for supply and two wires for the differential serial interface. One of the serial wires is also overlayed with the SDI-12 data wire. The sensor recognizes a command depending on the protocol that is used to issue a command. Instead of SDI-12, RS-485 uses two dedicated wires for the data signal. This allows the use of longer cables and is more insensitive to interference from outside sources, since the signal is related to the different wires, and supply currents do not influence the data signal. See [Wikipedia](#) for more details on RS-485.

TENSIOLINK RS-485 INTRODUCTION

tensioLINK is a fast, reliable, proprietary serial communications protocol that communicates over the RS-485 interface. This protocol is used to read out data and configure features of the device. METER provides a tensioLINK PC USB converter and software to communicate directly with the sensor, read out data, and update the firmware. Please contact [Customer Support](#) for more information about tensioLINK.

MODBUS RTU RS-485 INTRODUCTION

Modbus RTU is a common serial communications protocol used by Programmable Logic Controllers (PLCs) or data loggers to communicate with all kinds of digital devices. The communication works over the physical RS-485 connection. The combination of RS-485 for the physical connection and Modbus as serial communications protocol allows fast and reliable data transfer for a high number of sensors connected to one serial bus wire. Use the following links for more Modbus information: [Wikipedia](#) and [modbus.org](#).

INTERFACING THE SENSOR TO A COMPUTER

The serial signals and protocols supported by the sensor require some type of interface hardware to be compatible with the serial port found on most computers (or USB-to-serial adapters). There are several SDI-12 interface adapters available in the marketplace; however, METER has not tested any of these interfaces and cannot make a recommendation as to which adapters work with METER sensors. METER data loggers and the ZSC handheld device can operate as a computer-to-sensor interface for making on-demand sensor measurements.

TEROS 31 can also be configured and measured via tensioLINK using METER software tensioVIEW. To connect a TEROS 31 to a computer a tensioLINK USB converter and a suitable adapter cable is necessary.

BARO MODULE

The TEROS 31 in combination with a non-METER data logger needs a highly accurate barometric compensation to get the most precise soil water potential measurement. The BARO Module is an atmospheric pressure sensor that can use different connectors allowing it to be directly connected between a TEROS 31 and a data logger. The BARO Module can also be used as a stand-alone sensor for measuring atmospheric pressure. It can also act as a digital/analog converter to connect a tensiometer (TEROS 31) with serial output to a data logger with analog input channels. The logger obtains a barometric compensated analog metric potential signal. The BARO Module can be used for varied logger communications: SDI-12, Modbus, tensioLINK, analog voltage signal.

BAROMETRIC COMPENSATION

TEROS 31 measures the sum of matric potential and atmospheric pressure potential ($\Psi_p + \Psi_m$). To extract the matric potential, the barometric pressure should also be registered with a reference sensor. METER ZL6 and EM60 data loggers include a barometric pressure sensor and convert the signal into soil water potential. One atmospheric pressure sensor at every measuring site is enough to convert all TEROS 31 measurements at the site.

If using a non-METER data logger, a barometric sensor is needed at the measuring site. A barometric sensor (BARO Module) is available from METER by contacting [Customer Support](#).

Accounting for the barometric pressure after data collection can also be completed by subtracting atmospheric pressure from the TEROS 31 reading (P_{abs}):

$$\Psi_m = (P_{abs}) - P_a \quad \text{Equation 1}$$

METER SDI-12 IMPLEMENTATION

METER sensors use a low-impedance variant of the SDI-12 standard sensor circuit ([Figure 2](#)). During the power-up time, sensors output some sensor diagnostic information and should not be communicated with until the power-up time has passed. After the power up time, the sensors are fully compatible with all commands listed in the [SDI-12 Specification v1.3](#) except for the continuous measurement commands ([aR0 – aR9](#) and [aRC0 – aRC9](#)). [M](#), [R](#), and [C](#) command implementations are found on pages [8–9](#).

Out of the factory, all METER sensors start with SDI-12 address [0](#) and print out the DDI serial startup string during the power-up time. This can be interpreted by non-METER SDI-12 sensors as a pseudo-break condition followed by a random series of bits.

The TEROS 31 will omit the DDI serial startup string when the SDI-12 address is nonzero. Changing the address to a nonzero address is recommended for this reason.

SENSOR BUS CONSIDERATIONS

SDI-12 sensor buses require regular checking, sensor upkeep, and sensor troubleshooting. If one sensor goes down, that may take down the whole bus even if the remaining sensors are functioning normally. Power cycling the SDI-12 bus when a sensor is failing is acceptable. METER SDI-12 sensors can be power-cycled and read on the desired measurement interval or powered continuously and commands sent when a measurement is desired based on specified communication timing. Many factors influence the effectiveness of the bus configuration. Visit metergroup.com for articles and virtual seminars containing more information.

SDI-12 CONFIGURATION

Table 1 lists the SDI-12 communication configuration.

Table 1 SDI-12 communication configuration

Baud Rate	1,200
Start Bits	1
Data Bits	7 (LSB first)
Parity Bits	1 (even)
Stop Bits	1
Logic	Inverted (active low)

SDI-12 TIMING

All SDI-12 commands and responses must adhere to the format in Figure 4 on the data line. Both the command and response are preceded by an address and terminated by a carriage return and line feed combination (<CR><LF>) and follow the timing shown in Figure 5.

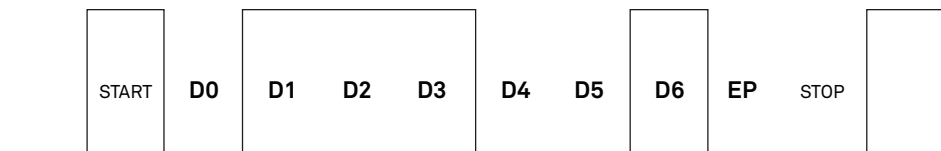


Figure 4 Example SDI-12 transmission of the character 1 (0x31)

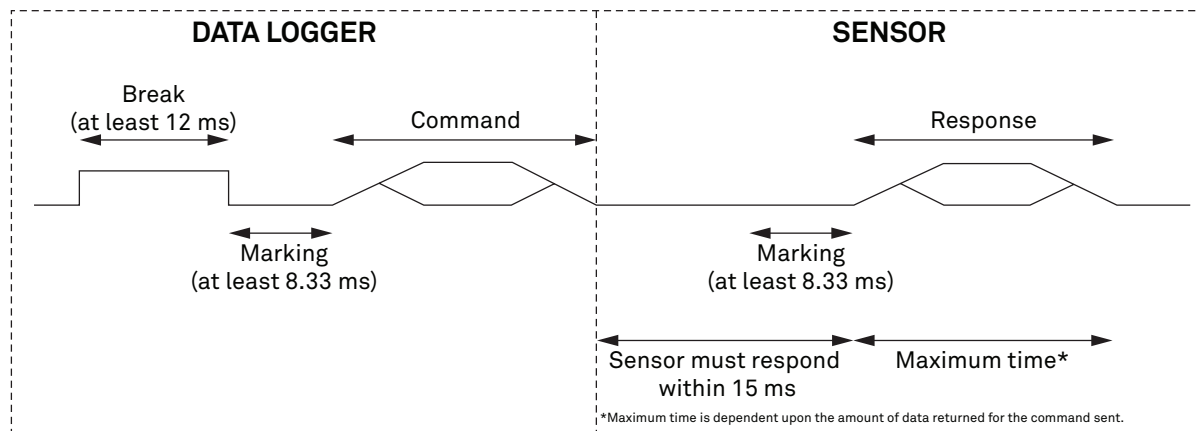


Figure 5 Example data logger and sensor communication

COMMON SDI-12 COMMANDS

This section includes tables of common SDI-12 commands that are often used in an SDI-12 system and the corresponding responses from METER sensors.

IDENTIFICATION COMMAND (**aI!**)

The Identification command can be used to obtain a variety of detailed information about the connected sensor. An example of the command and response is shown in Example 1, where the command is in **bold** and the response follows the command.

Example 1 1I!113METER_ _ _TER31_

Parameter	Fixed Character Length	Description
1I!	3	Data logger command. Request to the sensor for information from sensor address 1.
1	1	Sensor address. Prepended on all responses, this indicates which sensor on the bus is returning the following information.
13	2	Indicates that the target sensor supports SDI-12 Specification v1.3 .
METER_ _ _	8	Vendor identification string. (METER and three spaces _ _ _ for all METER sensors)
TER31_	6	Sensor model string. This string is specific to the sensor type. For the TEROS 31, the string is TER31.
100	3	Sensor version. This number divided by 100 is the METER sensor version (e.g., 100 is version 1.00).
T31-00001	≤13, variable	Sensor serial number. This is a variable length field. It may be omitted for older sensors.

CHANGE ADDRESS COMMAND (aAB!)

The Change Address command is used to change the sensor address to a new address. All other commands support the wildcard character as the target sensor address except for this command. All METER sensors have a default address of 0 (zero) out of the factory. Supported addresses are alphanumeric (i.e., A–Z, and 0–9). An example output from a METER sensor is shown in [Example 2](#), where the command is in **bold** and the response follows the command.

Example 2 1A0!0

Parameter	Fixed Character Length	Description
1A0!	4	Data logger command. Request to the sensor to change its address from 1 to a new address of 0.
0	1	New sensor address. For all subsequent commands, this new address will be used by the target sensor.

ADDRESS QUERY COMMAND (?!)

While disconnected from a bus, the Address Query command can be used to determine which sensors are currently being communicated with. Sending this command over a bus will cause a bus contention where all the sensors will respond simultaneously and corrupt the data line. This command is helpful when trying to isolate a failed sensor. [Example 3](#) shows an example of the command and response, where the command is in **bold** and the response follows the command. The question mark (?) is a wildcard character that can be used in place of the address with any command except the Change Address command.

Example 3 ?!0

Parameter	Fixed Character Length	Description
?!	2	Data logger command. Request for a response from any sensor listening on the data line.
0	1	Sensor address. Returns the sensor address to the currently connected sensor.

COMMAND IMPLEMENTATION

The following tables list the relevant Measurement (M), Continuous (R), and Concurrent (C) commands and subsequent Data (D) commands, when necessary.

MEASUREMENT COMMANDS IMPLEMENTATION

Measurement (M) commands are sent to a single sensor on the SDI-12 bus and require that subsequent Data (D) commands are sent to that sensor to retrieve the sensor output data before initiating communication with another sensor on the bus.

Please refer to [Table 2](#) and for an explanation of the command sequence and to [Table 5](#) for an explanation of response parameters.

Table 2 **aM!** command sequence

Command	Response
This command reports average, accumulated, or maximum values.	
aM!	atttn
aD0!	a±<Press>±<Temp>+<Status>
Comments	For a correct water potential measurement, a separate barometric (reference) pressure sensor is needed.

NOTE: The measurement and corresponding data commands are intended to be used back to back. After a measurement command is processed by the sensor, a service request a <CR><LF> is sent from the sensor signaling the measurement is ready. Either wait until **ttt** seconds have passed or wait until the service request is received before sending the data commands. See the [SDI-12 Specifications v1.3](#) document for more information.

CONCURRENT MEASUREMENT COMMANDS IMPLEMENTATION

Concurrent Measurement (C) commands are typically used with sensors connected to a bus. C commands for this sensor deviate from the standard C command implementation. First, send the C command, wait the specified amount of time detailed in the C command response, and then use D commands to read its response prior to communicating with another sensor.

Please refer to [Table 3](#) for an explanation of the command sequence and to [Table 5](#) for an explanation of response parameters.

Table 3 **aC!** measurement command sequence

Command	Response
This command reports instantaneous values.	
aC!	atttnn
aD0!	a±<Press>±<Temp>+<Status>

NOTE: Please see the [SDI-12 Specifications v1.3](#) document for more information.

CONTINUOUS MEASUREMENT COMMANDS IMPLEMENTATION

Continuous Measurement (R) commands trigger a sensor measurement and return the data automatically after the readings are completed without needing to send a D command.

aR0! returns more characters in its response than the 75-character limitation called out in the [SDI-12 Specification v1.3](#). It is recommended to use a buffer that can store at least 116 characters.

Please refer to [Table 4](#) for an explanation of the command sequence and see [Table 5](#) for an explanation of response parameters.

Table 4 **aR0!** measurement command sequence

Command	Response
This command reports average, accumulated, or maximum values.	
aR0!	a±<Press>±<Temp>+<Status>

NOTE: This command does not adhere to the SDI-12 response timing. See [METER SDI-12 Implementation](#) for more information.

PARAMETERS

Table 5 lists the parameters, unit measurement, and a description of the parameters returned in command responses for TEROs 31.

Table 5 Parameter Descriptions

Parameter	Unit	Description
$\pm$	—	Positive or negative sign denoting sign of the next value
a	—	SDI-12 address
n	—	Number of measurements (fixed width of 1)
nn	—	Number of measurements with leading zero if necessary (fixed width of 2)
ttt	s	Maximum time measurement will take (fixed width of 3)
<TAB>	—	Tab character
<CR>	—	Carriage return character
<LF>	—	Line feed character
<sensorType>	—	ASCII character denoting the sensor type For TEROs 31, the character is ;
<Checksum>	—	METER serial checksum
<CRC>	—	METER 6-bit CRC
<status>	—	<status> is sometimes returned with the D0 command but has no function and it will always return a value of 1.

DDI SERIAL COMMUNICATION

The DDI serial communications protocol is ideal for systems that have dedicated serial signaling lines for each sensor or use a multiplexer to handle multiple sensors. The serial communications are compatible with many TTL serial implementations that support active-high logic levels using 0- to 3.6-V signal levels. When the sensor is first powered, it automatically makes measurements of the integrated transducers then outputs a response over the data line. Systems using this protocol control the sensor excitation to initiate data transfers from the sensor. This protocol is subject to change as METER improves and expands the line of digital sensors and data loggers.

The TEROs 31 will omit the DDI serial startup string when the SDI-12 address is nonzero.

NOTE: Out of the factory, all METER sensors start with SDI-12 address 0 and print out the startup string when power cycled.

DDI SERIAL TIMING

Table 6 lists the DDI serial communication configuration.

Table 6 DDI serial communication configuration

Baud Rate	1,200
Start Bits	1
Data Bits	8 (LSB first)
Parity Bits	0 (none)
Stop Bits	1
Logic	Standard (active high)

At power up, the sensor will pull the data line high within 100 ms to indicate that the sensor is taking a reading (Figure 6). When the reading is complete, the sensor begins sending the serial signal out the data line adhering to the format shown in Figure 7. Once the data is transmitted, the sensor goes into SDI-12 communication mode. To get another serial signal, the sensor must be power cycled.

NOTE: Sometimes the signaling from the sensor can confuse typical microprocessor UARTs. The sensor holds the data line low while taking measurements. The sensor raises the line high to signal the logger that it will send a measurement. Then the sensor may take some additional measurements before starting to clock out the first data byte starting with a typical start bit (low). Once the first start bit is sent, typical serial timing is valid; however, the signal transitions before this point are not serial signaling and may be misinterpreted by the UART.

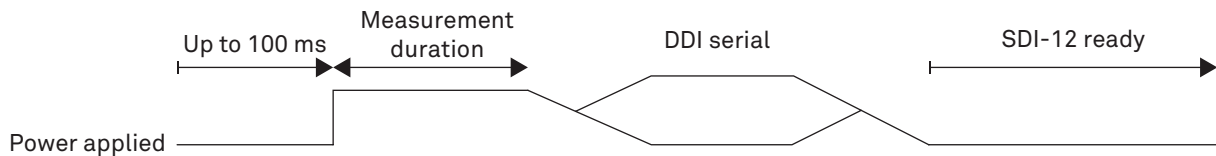


Figure 6 Data line DDI serial timing

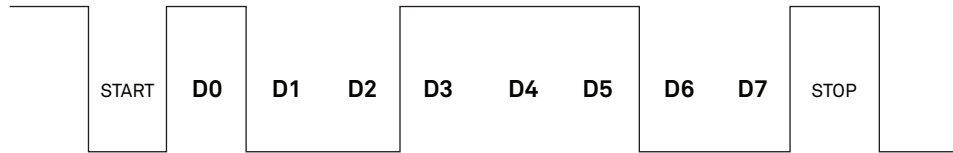


Figure 7 Example DDI serial transmission of the character 9 (0x39)

DDI SERIAL RESPONSE

Table 7 details the DDI serial response.

Table 7 DDI serial response

Command	Response
NA	<TAB><Press> <Temp> <METABITFIELD><CR><sensorType><Checksum><CRC>

NOTE: There is no actual command. The response is returned automatically upon power up.

DDI SERIAL CHECKSUM

These checksums are used in the DDI serial response. The legacy checksum is computed from the start of the transmission to the sensor identification character, excluding the sensor address.

Example input is <TAB>0<CR>]M and the resulting checksum output is x.

```
uint8_t LegacyChecksum(const char * response)
{
    uint16_t length;
    uint16_t i;
    uint16_t sum = 0;

    // Finding the length of the response string
    length = strlen(response);

    // Adding characters in the response together
    for(i = 0; i < length; i++)
    {
        sum += response[i];
        if(response[i] == '\r')
        {
            // Found the beginning of the metadata section of the response
            break;
        }
    }

    // Include the sensor type into the checksum
    sum += response[++i];

    // Convert checksum to a printable character
    sum = sum % 64 + 32;

    return sum;
}
```

The more robust CRC6 utilizes the CRC-6-CDMA2000-A polynomial with the value 48 added to the results to make this a printable character and is computed from the start of the transmission to the legacy checksum character, excluding the sensor address.

CRC6 checksum example input is <TAB>1.222 23.4 92.81<CR>{/6 and the resulting checksum output is x.

```
uint8_t CRC6_Offset(const char *buffer)
{
    uint16_t byte;
    uint16_t i;
    uint16_t bytes;
    uint8_t bit;
    uint8_t crc = 0xfc; // Set upper 6 bits to 1's

    // Calculate total message length—updated once the metadata section is found
    bytes = strlen(buffer);

    // Loop through all the bytes in the buffer
    for(byte = 0; byte < bytes; byte++)
    {
        // Get the next byte in the buffer and XOR it with the crc
        crc ^= buffer[byte];

        // Loop through all the bits in the current byte
        for(bit = 8; bit > 0; bit--)
        {
            // If the uppermost bit is a 1...
            if(crc & 0x80)
            {
                // Shift to the next bit and XOR it with a polynomial
                crc = (crc << 1) ^ 0x9c;
            }
            else
            {
                // Shift to the next bit
                crc = crc << 1;
            }
        }
        if(buffer[byte] == '\r')
        {
            // Found the beginning of the metadata section of the response
            // both sensor type and legacy checksum are part of the crc6
            // this requires only two more iterations of the loop so reset
            // "bytes"

            // bytes is incremented at the beginning of the loop, so 3 is added
            bytes = byte + 3;
        }
    }

    // Shift upper 6 bits down for crc
    crc = (crc >> 2);

    // Add 48 to shift crc to printable character avoiding \r \n and !
    return (crc + 48);
}
```

METER MODBUS RTU SERIAL IMPLEMENTATION

Modbus over Serial Line is specified in two versions - ASCII and RTU. METER TEROS 31 sensors communicate using RTU mode exclusively. The following explanation is always related to RTU. Table 8 lists the Modbus RTU communication and configuration.

Table 8 Modbus communication characters

Baud Rate (bps)	9,600 bps
Start Bits	1
Data Bits	8 (LSB first)
Parity Bits	0 (none)
Stop Bits	1
Logic	Standard (active high)

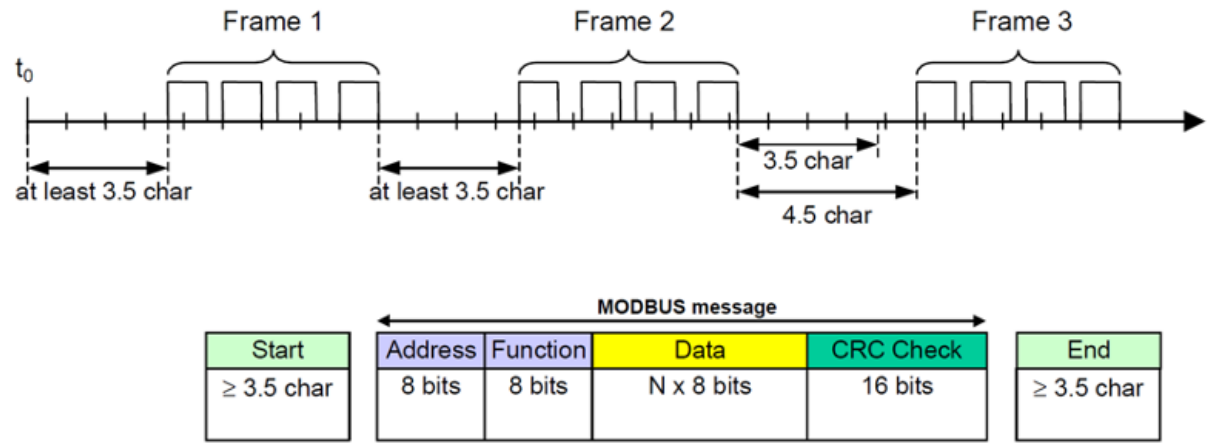
**Figure 8 RTU Message Frame**

Figure 8 shows a message in RTU format. The size of the data determines the length of the message. The format of each byte in the message has 10 bits, including Start and Stop Bit. Each byte is sent from left to right: Least Significant Bit (LSB) to Most Significant Bit (MBS). If no parity is implemented, an additional stop bit is transmitted to fill out the character frame to a full 11-bit asynchronous character.

The Modbus application layer implements a set of standard Function codes divided into three categories: Public, User-defined, and Reserved. Well-defined public function codes for TEROS sensors are documented in the Modbus Organization, Inc. (modbus.org) community.

For a reliable interaction between the TEROS sensors and a Modbus Master, a **minimum 50ms** delay is required between every Modbus command sent on the RS-485 bus. An additional timeout is needed for every Modbus query; this timeout is device-specific and depends on the quantity of the polled registers. Generally, **100ms** will work fine for most of the TEROS sensors.

SUPPORTED MODBUS FUNCTIONS

Table 9 Function Definitions

Function Code	Action	Description
01	Read coil/port status	Reads the on/off status of discrete output(s) in the ModBusSlave
02	Read input status	Reads the on/off status of discrete input(s) in the ModBusSlave
03	Read holding registers	Reads the binary contents of holding register(s) in the ModBusSlave
04	Read input registers	Reads the binary contents of input register(s) in the ModBusSlave
05	Force single coil/port	Forces a single coil/port in the ModBusSlave to either on or off
06	Write single register	Writes a value into a holding register in the ModBusSlave
15	Force multiple coils/ports	Forces multiple coils/ports in the ModBusSlave to either on or off
16	Write multiple registers	Writes values into a series of holding registers in the ModBusSlave

DATA REPRESENTATION AND REGISTER TABLES

Data values (setpoint values, parameters, sensor-specific measurement values, etc.) sent to and from the TEROS sensors use 16-bit and 32-bit holding (or input) registers with a 4-digit address notation. The address spaces are virtually distributed in different blocks for each data type. This is an approach to the Modbus Enron implementation. [Table 10](#) shows the four main tables used by the TEROS sensors with their respective access rights. [Table 11](#) describes the sub-blocks for each different data type representation.

Please note that some Modbus dataloggers use addressing with a +1 offset. This sometimes causes confusion and is based on a Modbus specification void. If there are problems in implementing your Modbus program on the datalogger always try testing different register offsets and data types. Using a known value, like temperature, where it's known what value to expect is a good practice to start testing.

Table 10 Modbus Primary Tables

Register Number	Table Type	Access	Description
1xxx	Discrete Output Coils	Read/Write	on/off status or setup flags for the sensor
2xxx	Discrete Input Contacts	Read	sensor status flags
3xxx	Analog Input Registers	Read	numerical input variables from the sensor (actual sensor measurements)
4xxx	Analog Output Holding Registers	Read/Write	numerical output variables for the sensor (parameters, setpoint values, calibrations etc.)

For example, register 3001 is the first analog input register (first data address for the input registers). The numeric value stored here would be a 16-bit unsigned integer-type variable that represents the first sensor measurement parameter (pressure value). The same measurement parameter (pressure value) could be read at register 3201, but this time as a 32-bit floating-point value with a Big-Endian format. If the Modbus Master (Datalogger or a PLC) supports only 32-bit float-values with a Little-Endian format, then one could read the same measurement parameter (same pressure value) at register 3301. The Virtual Sub-Blocks are meant to simplify the user's effort in programming the Modbus query of the sensors.

Table 11 Modbus Virtual Sub-Blocks

Register Number	Access	Size	Sub-Table Data Type
X001-X099	Read/Write	16 bit	signed integer
X101-X199	Read/Write	16 bit	unsigned integer
X201-X299	Read/Write	32 bit	float Big-Endian format
X301-X399	Read/Write	32 bit	float Little-Endian format

REGISTER MAPPING

Table 12 Holding Registers

4100 (4101*)	Modbus Slave Address
Detailed Description	Read or update the sensor's modbus address
Data Type	Unsigned integer
Allowed Range	1 - 247
Unit	-
Comments	Updated slave address will be stored in the sensor's nonvolatile memory

Table 13 Teros 31 Input Registers

3200 (3201*)	Soil Water Potential
Detailed Description	Absolute pressure value
Data Type	32 bit floating Big-Endian
Allowed Range	-200 to +200
Unit	kPa
Comments	For a correct water potential measurement, a separate barometric (reference) pressure sensor is needed . Refer to Barometric compensation on page 5 .
3201 (3202*)	Soil Temperature
Detailed Description	High accuracy on board temperature measurement
Data Type	32 bit floating Big-Endian
Allowed Range	-30 to +60
Unit	degC
Comments	-
3202 (3203*)	Sensor Supply Voltage
Detailed Description	On board supply voltage measurement
Data Type	32 bit floating Big-Endian
Allowed Range	-10 to +60
Unit	Volts
Comments	-
3203 (3204*)	Installation Pitch Angle
Detailed Description	Tensiometer installation pitch angle
Data Type	32 bit floating Big-Endian
Allowed Range	-180 to +180
Unit	deg
Comments	Sensor failure will output a 9999 value
3204 (3205*)	Installation Roll Angle
Detailed Description	Tensiometer installation roll angle
Data Type	32 bit floating Big-Endian
Allowed Range	-90 to +90
Unit	deg
Comments	Sensor failure will output a 9999 value

*Some devices report Modbus register addresses with an offset of +1. This is true for Campbell Scientific Loggers and Datataker loggers. In order to read the desired register use the number in the parenthesis.

EXAMPLE USING A CR6 DATALOGGER AND MODBUS RTU

The Campbell Scientific, Inc. CR6 Measurement and Control Datalogger supports Modbus master and Modbus slave communication to integrate Modbus SCADA networks. The Modbus communications protocol facilitates the exchange of information and data between a computer/HMI software, instruments

(RTUs), and Modbus-compatible sensors. The CR6 datalogger communicates exclusively in RTU mode. In a Modbus network, each slave device has a unique address. Therefore, sensor devices must be configured correctly before connecting to a Modbus Network. Addresses range from 1 to 247. Address 0 is reserved for universal broadcasts.

PROGRAMMING A CR6 DATALOGGER

The Programs running on the CR6 (and CR1000) Loggers are written in CRBasic, a language developed by Campbell Scientific. It is a high-level language designed to provide an easy yet extremely flexible and powerful method of instructing the data logger how and when to take measurements, process data, and communicate. Programs can be created using either the ShortCut Software or edited using the CRBasic Editor, both of which are available for downloading as stand-alone applications on the official [Campbell Scientific website](http://www.campbellsci.com) (www.campbellsci.com).

[ShortCut Software](https://www.campbellsci.com/shortcut) (<https://www.campbellsci.com/shortcut>)

[CRBasic Editor](https://www.campbellsci.com/crbasiceditor) (<https://www.campbellsci.com/crbasiceditor>)

A typical CRBasic program for a Modbus application consists of the following:

- Variables and constants declarations (public or private)
- Units declarations
- Configuration parameters
- Data tables declarations
- Logger Initializations
- Scan (Main Loop) with all the sensors to be quired
- Function call to the Data Tables

CR6 LOGGER RS-485 CONNECTION INTERFACE

The universal (U) terminal of the CR6 offers 12 Channels that connect to nearly any sensor type. It gives the CR6 the ability to match more applications and eliminates the use of many external peripherals.

The Modbus CR6 connection shown in [Figure 9](#) uses the RS-485 (A/B) interface mounted on terminals (C1-C2) and (C3-C4). These interfaces can operate in Half-Duplex and Full-Duplex. The serial interface of the TEROS Sensor used for this example is connected to (C1-C2) terminals.

TEROS 31 to CR6 Datalogger Wiring Diagram

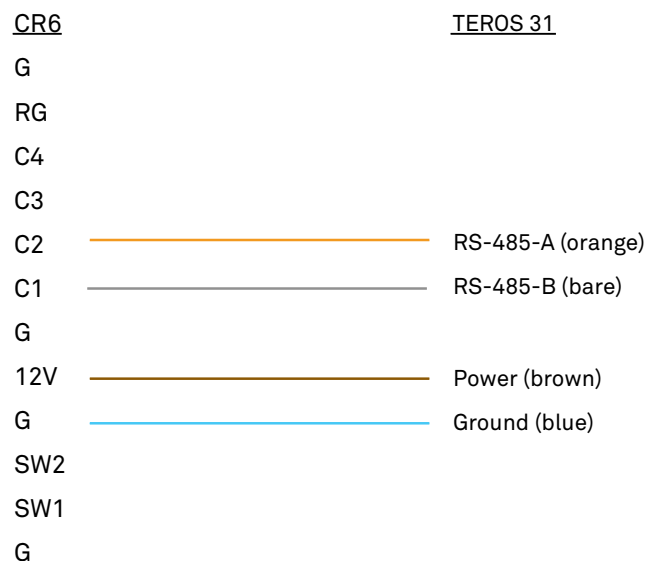


Figure 9 RS-485 interface

After assigning the TEROS sensor a unique Modbus Slave Address, it can be wired to the CR6 logger according to [Figure 9](#). Make sure to connect the orange and bare wires according to their signals, respectively, to the C1 and C2 ports—the brown wire to 12V (V+) and the blue to G (GND). To control the power supply through your program, connect the brown wire directly to one of the SW12 terminals (switched 12V outputs).

EXAMPLE PROGRAMS

```

'CR6 Datalogger
'This is an example program for reading out the Teros31 Tensiometer using a CR6
'datalogger and the MODBUS RTU protocol over a RS-485 Bus. The measurement values polled
'from the sensor will be: Water Potential, Temperature and the Sensor's Supply voltage.

'This program runs a scan every 1 Min and stores the data in a 1 Min table.

'Declare Constants
Const TEROS_MB_ADDR=1      'Teros31 Modbus slave address
Const MB_TIMEOUT= 10      '100ms timeout (value * 0.01sec)
Const MB_RETRIES= 1

'Declare Public Variables
Public PTemp, batt_volt
Public mb_statu 'variable used for monitoring the modbus poll status

'Declare Private Variables
Dim Measurements (3) 'array for holding the measurements values read from the sensor

'Aliases used for the TEROS 31-32
Alias Measurements (1)= Water Potential
Alias Measurements (2)= Temperature
Alias Measurements (3)= Sensor Supply

'Declare Units
Units Water Potential=hPa
Units Temperature=degC
Units Sensor supply=V

'Define Data Tables.
DataTable (Teros_Table,1,-1) 'Set table size to # of records, or -1 to auto allocate.
DataInterval (0,1,Min,10) 'Store new measurement every 1 Minute
Minimum (1,batt_volt,FP2,False,False)
Sample (1,PTemp,FP2)
Sample (3,Measurements(),IEEE4)

EndTable

'Main Program

BeginProg

SW12(2,1) 'Switch ON the SW12-2 terminal (if used for powering the Teros sensor)

SerialOpen(ComC1,9600,3,2,50,4) 'open communication port, setup for RS-485
'(BaudRate, Format, TXDelay, BufferSize, CommsMode)

Scan (1,Min,0,0) 'Scan Loop
PanelTemp (PTemp,15000)
Battery (batt_volt)

'Read multiple Input registers from the Teros sensors using a 32 bit float, Big-Endian
'format
ModbusMaster(mb_status,ComC1,9600,TEROS_MB_ADDR,4,Measurements(),3201,3,MB_RETRIES,MB_
TIMEOUT,2)

'Call Output Tables
CallTable Teros_Table

NextScan

EndProg

```

CUSTOMER SUPPORT

EUROPE

Customer service representatives are available for questions, problems, or feedback Monday through Friday, 8:00 to 17:00 Central European time.

Email: support.europe@metergroup.com
sales.europe@metergroup.com

Phone: +49 89 12 66 52 0

Fax: +49 89 12 66 52 20

Website: metergroup.com

NORTH AMERICA

Customer service representatives are available for questions, problems, or feedback Monday through Friday, 7:00 am to 5:00 pm Pacific time.

Email: support.environment@metergroup.com
sales.environment@metergroup.com

Phone: +1.509.332.5600

Fax: +1.509.332.5158

Website: metergroup.com

If contacting METER by email, please include the following information:

Name	Email address
Address	Instrument serial number
Phone number	Description of problem

NOTE: For products purchased through a distributor, please contact the distributor directly for assistance.

REVISION HISTORY

The following table lists document revisions.

Revision	Date	Compatible Firmware	Description
10	4.2026	2.5.0	Updated Table 5, the parameters returned in command responses for TEROs 31.
09	3.2026	2.5.0	Barometric pressure compensation information, equation, and IP rating
08	3.2025	2.5.0	SDI-12 power cycle information modified
07	11.2024	2.5.0	Modbus register update and BARO module added
06	5.2024	2.5.0	Modbus information added
05	4.2024	1.14	Updated 4-wire figure and information to be current
04	11.2023	1.14	Added info about outside barometric readings needed
03	7.2023	1.14	Updated company info, ISO status
02	3.2022	1.14	Updated boot loader function
01	12.2021	1.00	Corrected checksum and specifications
00	1.2021	1.00	Initial release